

## KeyTec<sup>®</sup> Renilla


### Luciferase Detection Kit

#### Instruction Manual

#### 1. Introduction

KeyTec<sup>®</sup> Renilla luciferase Detection kit is designed for the sensitive and robust detection of Renilla luciferase reporter gene assays. Simply mix the substrate with cell lysis buffer, add the mixture to the cells, and proceed to detect the Renilla luciferase signal within the cells.

The detection principle is based on Luminescent technology. Within the kit, Coelenterazine reacts with Renilla luciferase released by cells, generating a sensitive and robust luminescence signal. The process provides a highly sensitive, robust, and homogeneous assay for the detection of Renilla luciferase reporter gene expression in mammalian cells. (Figure 1)

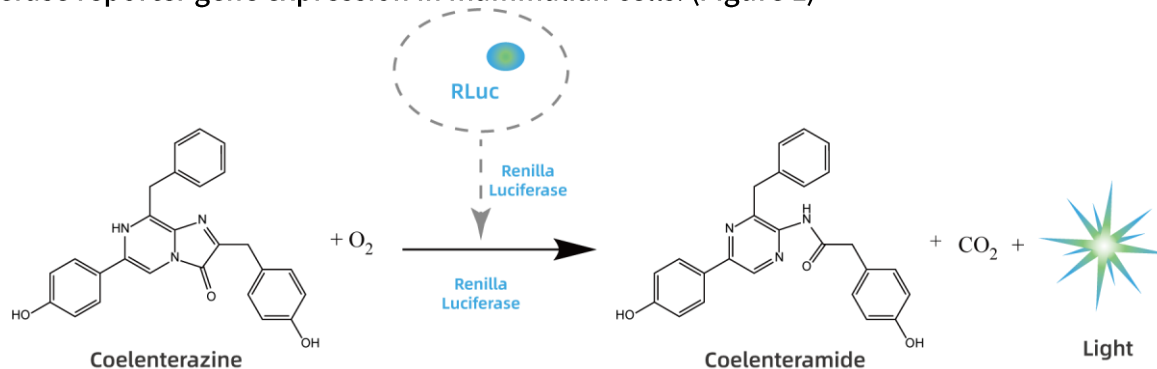

**Figure 1.** The Renilla luciferase reaction of KeyTec<sup>®</sup> luciferase detection kit

## 2. Components

CAT.	Description	Size
A2001100N	KeyTec® Renilla Luciferase Detection Kit (100 tests)	10 mL

Each kit contains sufficient reagents to perform 100 tests of 100 µL/well.

The kit contains the following components:

- 1 × 100 µL KeyTec® Renilla Luciferase Substrate 100X
- 1 × 10 mL KeyTec® Renilla Luciferase Cell lysis buffer

CAT.	Description	Size
A2001100N	KeyTec® Renilla Luciferase Detection Kit (1,000 tests)	2*50 mL

Each kit contains sufficient reagents to perform 1,000 tests of 100 µL/well.

The kit contains the following components:

- 2 × 500 µL KeyTec® Renilla Luciferase Substrate 100X
- 2 × 50 mL KeyTec® Renilla Luciferase Cell lysis buffer

CAT.	Description	Size
A2001100N	KeyTec® Renilla Luciferase Detection Kit (5,000 tests)	2*250 mL

Each kit contains sufficient reagents to perform 5,000 tests of 100 µL/well.

The kit contains the following components:

- 4 × 1.25 mL KeyTec® Renilla Luciferase Substrate 100X
- 2 × 250 mL KeyTec® Renilla Luciferase Cell lysis buffer

## 3. Storage Conditions

- ◆ Upon receipt, store the kit below -20 °C. While it can be stored for an extended period, we recommend using it within the specified validity period (refer to the CoA for details).
- ◆ The kit can withstand up to 10 cycles of freezing and thawing (≥90% activity).
- ◆ When first thaw, aliquot the reagents as needed to avoid multiple freeze-thaw cycles.
- ◆ We recommend preparing the mixed reagent immediately before use. Discard any remaining substrate detection solution after the assay; do not store it.

## 4. Materials Required But Not Supplied

Materials	Recommended Brand	CAT.
Cell Culture Plate (96-well, clear flat bottom, white)	Corning	3610
	Greiner	655098
White Microplates Bottom Seals	VKEY-BIO	M1000302N
Pipettes	Multiple Choices	\
Microplate Shakers	Multiple Choices	\
Microplate Reader With Luminescence	Multiple Choices	\

## 5. Assay Procedure

Procedure	Stage	Operation
Step 1	Reagents Preparation	<ul style="list-style-type: none"> <li>➤ <b>Melt the reagents:</b> Allow the Substrate and Cell Lysis Buffer to thaw at room temperature (not above 25 °C) before use.</li> <li>➤ <b>Centrifuge after equilibration:</b> After the reagents have equilibrated to room temperature, it is recommended to centrifuge the bottles before opening the lids to concentrate the liquid at the bottom.</li> <li>➤ <b>Prepare mixed reagent:</b> mix the "KeyTec® Renilla Luciferase Substrate 100X" with the "KeyTec® Renilla Luciferase Cell Lysis Buffer" using a 1:100 volume ratio. Ensure thorough mixing to achieve the required volume of detection reagent.</li> </ul>
Step 2	Detection	<ul style="list-style-type: none"> <li>➤ <b>Equilibrate culture plate temperature:</b> Equilibrate the cell culture plate to room temperature.</li> <li>➤ <b>Add reagent:</b> Add an equal volume of premixed detection reagent to the sample to be tested. (It is recommended to add 100 µL of premixed reagent to 100 µL of the cell culture to be tested.)</li> <li>➤ <b>Shake the plate:</b> Shake the plate at 1200 rpm for 5 minutes. Full shaking enhances the effect, ensuring thorough cell lysis and mixing.</li> <li>➤ <b>Read Signal:</b> Read the luminescence signal with a microplate reader.</li> </ul>

Note: PBS buffer can inhibit firefly luciferase activity leading to low signal values, and PBS buffer should be avoided in the final test samples.

## 6. Performance

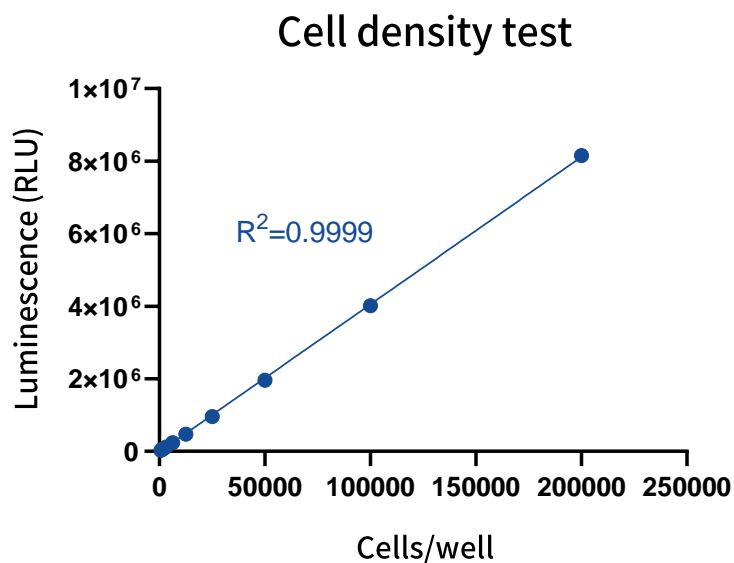


Figure 2. Correlation between Cell Number and Luminescence

Use KeyTec® Renilla Luciferase Detection Kit to detect the overexpression of Renilla luciferase in the HEK293 cell line. The results showed a linear relationship between the luminescence signal and the number of cells. HEK293 cells, cultured in DMEM medium with 10% FBS, were serially diluted two-fold, starting from 50,000 cells per well in a 96-well plate. Perform the assay according to the procedure outlined in Section 5. “Assay Procedure”. Five minutes after adding the reagent, measure the luminescence signal using the Envision's Luminescence program. (Example program details include Mirror: Luminescence, Em filter: Luminescence 700, Measurement height: 6.5 mm, and Measurement time: 1 s).

**Tip:** The data provided above is for reference only. Actual results may vary depended on the performance of the microplate reader used.